

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0069
Location:	MARLBORO TWP. POLICE	
Calibration File No.:	00368	Calib. Date: 10/12/2012
Certification File No.:	00369	Calib. No.: 00018
Linearity File No.:	00371	Cert. Date: 10/12/2012
Solution File No.:	00382	Cert. No.: 00011
Sequential File No.:	00382	Lin. Date: 10/12/2012
		Lin. No.: 00014
		Soln. Date: 12/13/2012
		Soln. No.: 00082
		File Date: 12/13/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0162
Solution Control Lot:	12F102	Expires: 06/28/2014
		Bottle No.: 0377

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:47S		
Control 1 EC	0.099%	11:47S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:48S		
Control 2 EC	0.098%	11:49S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:50S		
Control 3 EC	0.097%	11:50S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:51S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OHARE

First Name: BRYAN


MI: F

Signature: _____



Badge No.: 96

Date: 12/13/2012

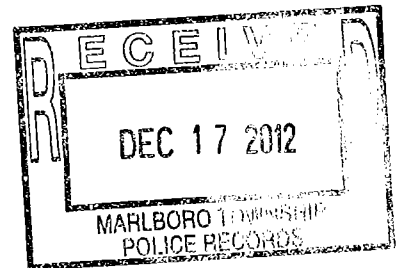

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0069
Location:	MARLBORO TWP. POLICE		
Calibration File No.:	00368	Calib. Date:	10/12/2012
Certification File No.:	00369	Cert. Date:	10/12/2012
Linearity File No.:	00371	Lin. Date:	10/12/2012
Solution File No.:	00381	Soln. Date:	12/13/2012
Sequential File No.:	00381	File Date:	12/13/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0162
Solution Control Lot:	12F102	Expires:	06/28/2014
		Bottle No.:	0377

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:03S		
Control 1 EC	0.099%	09:04S	34.0°C	AMBIENT AIR CHECK ERR
Control 1 IR	-.---%	09:04S	34.0°C	AMBIENT AIR CHECK ERR
Ambient Air Blank	-.---%	09:04S		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OHARE

First Name: BRYAN


MI: F

Signature: _____

Sgt. [Signature] #096

Badge No.: 96

Date: 12/13/2012

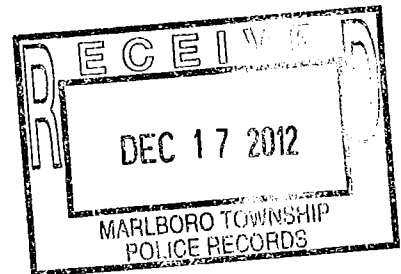

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0069
Location:	MARLBORO TWP. POLICE	
Calibration File No.:	00368	Calib. Date: 10/12/2012
Certification File No.:	00369	Calib. No.: 00018
Linearity File No.:	00371	Cert. Date: 10/12/2012
Solution File No.:	00378	Cert. No.: 00011
Sequential File No.:	00378	Lin. Date: 10/12/2012
		Lin. No.: 00014
		Soln. Date: 11/10/2012
		Soln. No.: 00080
		File Date: 11/10/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0162
Solution Control Lot:	12F102	Expires: 06/28/2014
		Bottle No.: 0376

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:47S		
Control 1 EC	0.099%	09:47S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:48S		
Control 2 EC	0.097%	09:49S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:49S		
Control 3 EC	0.098%	09:50S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:51S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OHARE

First Name: BRYAN


MI: F

Signature: _____

Sgt. Jim #096

Badge No.: 96

Date: 11/10/2012

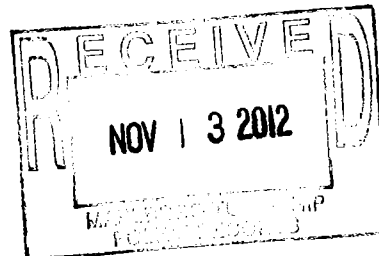

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0069
Location:	MARLBORO TWP. POLICE	
Calibration File No.:	00311	Calib. Date: 04/16/2012
Certification File No.:	00312	Calib. No.: 00016
Linearity File No.:	00313	Cert. Date: 04/16/2012
Solution File No.:	00363	Cert. No.: 00009
Sequential File No.:	00363	Lin. Date: 04/16/2012
		Lin. No.: 00011
		Soln. Date: 10/03/2012
		Soln. No.: 00078
		File Date: 10/03/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0164
Solution Control Lot:	11C088	Expires: 03/31/2013
		Bottle No.: 0145

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:19D		
Control 1 EC	0.099%	11:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:20D		
Control 2 EC	0.098%	11:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	11:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:22D		
Control 3 EC	0.098%	11:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OHARE

First Name: BRYAN

MI: F

Signature: _____

Sgt. [Signature] #056

Badge No.: 96

Date: 10/03/2012



Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0069
Location: MARLBORO TWP. POLICE
Calibration File No.: 00311 Calib. Date: 04/16/2012 Calib. No.: 00016
Certification File No.: 00312 Cert. Date: 04/16/2012 Cert. No.: 00009
Linearity File No.: 00313 Lin. Date: 04/16/2012 Lin. No.: 00011
Solution File No.: 00354 Soln. Date: 09/04/2012 Soln. No.: 00077
Sequential File No.: 00354 File Date: 09/04/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0164
Control Solution %: 0.100% Expires: 03/31/2013
Solution Control Lot: 11C088 Bottle No.: 0140

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:52D		
Control 1 EC	0.099%	20:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:53D		
Control 2 EC	0.099%	20:53D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:54D		
Control 3 EC	0.098%	20:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	20:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:55D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LAYMAN

First Name: JOSHUA

MI: E

Signature: _____

Badge No.: 101

Date: 09/04/2012

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0069
Location:	MARLBORO TWP. POLICE	
Calibration File No.:	00311	Calib. Date: 04/16/2012
Certification File No.:	00312	Calib. No.: 00016
Linearity File No.:	00313	Cert. Date: 04/16/2012
Solution File No.:	00352	Cert. No.: 00009
Sequential File No.:	00352	Lin. Date: 04/16/2012
		Lin. No.: 00011
		Soln. Date: 09/03/2012
		Soln. No.: 00076
		File Date: 09/03/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0164
Solution Control Lot:	11C088	Expires: 03/31/2013
		Bottle No.: 0130

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	03:42D		
Control 1 EC	0.099%	03:43D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:43D		
Control 2 EC	0.098%	03:44D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	03:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:44D		
Control 3 EC	0.097%	03:45D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	03:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:46D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LAYMAN

First Name: JOSHUA


MI: E

Signature: _____

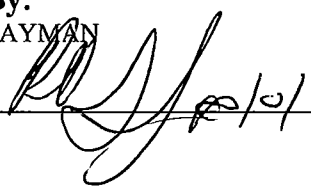

Badge No.: 101

Date: 09/03/2012

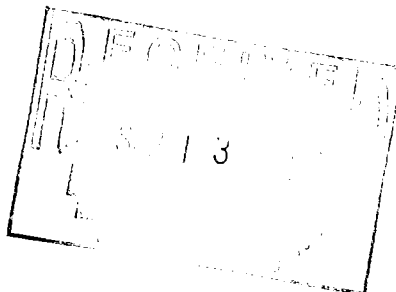

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0069		
Location:	MARLBORO TWP. POLICE				
Calibration File No.:	00311	Calib. Date:	04/16/2012	Calib. No.:	00016
Certification File No.:	00312	Cert. Date:	04/16/2012	Cert. No.:	00009
Linearity File No.:	00313	Lin. Date:	04/16/2012	Lin. No.:	00011
Solution File No.:	00351	Soln. Date:	09/03/2012	Soln. No.:	00075
Sequential File No.:	00351	File Date:	09/03/2012		
Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDXC S3-0164
Control Solution %:	0.100%			Expires:	03/31/2013
Solution Control Lot:	11C088			Bottle No.:	0130

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:29D		
Control 1 EC	-.---%	00:30D	23.6°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	00:30D	23.6°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	---:--		
Control 2 EC	-.---%	---:--	N/A	
Control 2 IR	-.---%	---:--	N/A	
Ambient Air Blank	-.---%	---:--		
Control 3 EC	-.---%	---:--	N/A	
Control 3 IR	-.---%	---:--	N/A	
Ambient Air Blank	-.---%	---:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LAYMAN

First Name: JOSHUA


MI: E

Signature: _____



Badge No.: 101

Date: 09/03/2012

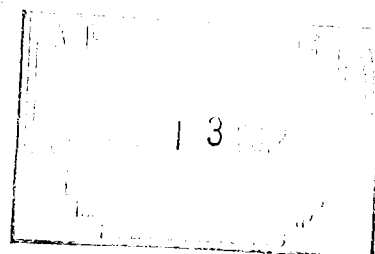

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0069
Location:	MARLBORO TWP. POLICE	
Calibration File No.:	00311	Calib. Date: 04/16/2012
Certification File No.:	00312	Calib. No.: 00016
Linearity File No.:	00313	Cert. Date: 04/16/2012
Solution File No.:	00350	Cert. No.: 00009
Sequential File No.:	00350	Lin. Date: 04/16/2012
		Lin. No.: 00011
		Soln. Date: 09/02/2012
		Soln. No.: 00074
		File Date: 09/02/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0164
Solution Control Lot:	11C088	Expires: 03/31/2013
		Bottle No.: 0135

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:27D		
Control 1 EC	-.---%	23:28D	24.9°C	SIMULATOR TEMP. ERROR
Control 1 IR	-.---%	23:28D	24.9°C	SIMULATOR TEMP. ERROR
Ambient Air Blank	-.---%	--:--		
Control 2 EC	-.---%	--:--	N/A	
Control 2 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		
Control 3 EC	-.---%	--:--	N/A	
Control 3 IR	-.---%	--:--	N/A	
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: LAYMAN

First Name: JOSHUA


MI: E

Signature: _____



Badge No.: 101

Date: 09/02/2012

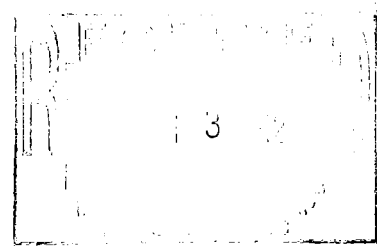

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0069
Location:	MARLBORO TWP. POLICE	
Calibration File No.:	00311	Calib. Date: 04/16/2012
Certification File No.:	00312	Calib. No.: 00016
Linearity File No.:	00313	Cert. Date: 04/16/2012
Solution File No.:	00338	Cert. No.: 00009
Sequential File No.:	00338	Lin. Date: 04/16/2012
		Lin. No.: 00011
		Soln. Date: 08/06/2012
		Soln. No.: 00073
		File Date: 08/06/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0164
Solution Control Lot:	11C088	Expires: 03/31/2013
		Bottle No.: 0129

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:56D		
Control 1 EC	0.099%	14:57D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	14:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:58D		
Control 2 EC	0.098%	14:58D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:59D		
Control 3 EC	0.098%	15:00D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	15:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:00D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: TOMAZIC

First Name: JOSEPH


MI: M

Signature: _____

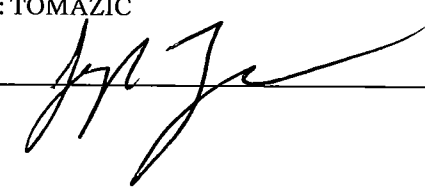

Badge No.: 085

Date: 08/06/2012

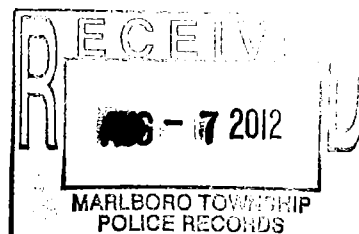

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0069
Location:	MARLBORO TWP. POLICE	
Calibration File No.:	00311	Calib. Date: 04/16/2012
Certification File No.:	00312	Calib. No.: 00016
Linearity File No.:	00313	Cert. Date: 04/16/2012
Solution File No.:	00333	Lin. No.: 00011
Sequential File No.:	00333	Soln. Date: 07/08/2012
		Soln. No.: 00072
		File Date: 07/08/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0164
Solution Control Lot:	11C088	Expires: 03/31/2013
		Bottle No.: 0134

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	02:48D		
Control 1 EC	0.098%	02:49D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	02:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:49D		
Control 2 EC	0.097%	02:50D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	02:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:51D		
Control 3 EC	0.097%	02:51D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	02:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:52D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OHARE

First Name: BRYAN


MI: F

Signature: _____

SA. [Signature] #096

Badge No.: 96

Date: 07/08/2012

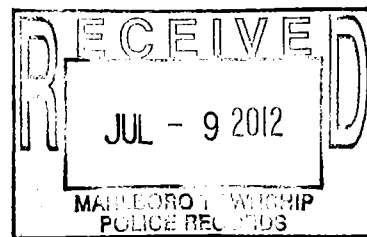

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0069
Location:	MARLBORO TWP. POLICE	Calib. No.:	00016
Calibration File No.:	00311	Cert. Date:	04/16/2012
Certification File No.:	00312	Lin. Date:	04/16/2012
Linearity File No.:	00313	Soln. Date:	06/14/2012
Solution File No.:	00325	File Date:	06/14/2012
Sequential File No.:	00325		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0164
Solution Control Lot:	11C088	Expires:	03/31/2013
		Bottle No.:	0139

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:48D		
Control 1 EC	0.099%	09:48D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:49D		
Control 2 EC	0.098%	09:50D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:50D		
Control 3 EC	0.098%	09:51D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	09:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:51D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OHARE

First Name: BRYAN


MI: F

Signature: _____

Sgt. [Signature] #096

Badge No.: 96

Date: 06/14/2012

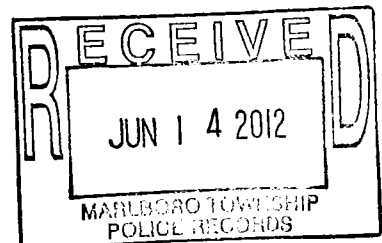

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0069
Location:	MARLBORO TWP. POLICE		
Calibration File No.:	00311	Calib. Date:	04/16/2012
Certification File No.:	00312	Cert. Date:	04/16/2012
Linearity File No.:	00313	Lin. Date:	04/16/2012
Solution File No.:	00316	Soln. Date:	05/16/2012
Sequential File No.:	00316	File Date:	05/16/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0164
Solution Control Lot:	11C088	Expires:	03/31/2013
		Bottle No.:	0149

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:58D		
Control 1 EC	0.099%	10:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	10:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:59D		
Control 2 EC	0.097%	10:59D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	10:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:00D		
Control 3 EC	0.097%	11:01D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:01D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OHARE

First Name: BRYAN

MI: F

Signature: _____



Badge No.: 96

Date: 05/16/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0069
Location:	MARLBORO TWP. POLICE	Calib. No.:	00016
Calibration File No.:	00311	Calib. Date:	04/16/2012
Certification File No.:	00312	Cert. No.:	00009
Linearity File No.:	00313	Lin. Date:	04/16/2012
Solution File No.:	00314	Soln. No.:	00069
Sequential File No.:	00314	File Date:	04/16/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0164
Solution Control Lot:	11C088	Expires:	03/31/2013
		Bottle No.:	0133

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:02D		
Control 1 EC	0.103%	12:03D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:04D		
Control 2 EC	0.102%	12:04D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:05D		
Control 3 EC	0.101%	12:06D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	12:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:06D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL # DDUJ P2-080 (MD)

Changed By:

Last Name: DENNIS

First Name: MARC

MI: W.

Signature: _____

TBR. I [Signature] Dennis #5925

Badge No.: 5925

Date: 04/16/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0069
Location:	MARLBORO TWP. POLICE		
Calibration File No.:	00261	Calib. Date:	11/01/2011
Certification File No.:	00262	Cert. Date:	11/01/2011
Linearity File No.:	00263	Lin. Date:	11/01/2011
Solution File No.:	00305	Soln. Date:	04/04/2012
Sequential File No.:	00305	File Date:	04/04/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0162
Solution Control Lot:	11C088	Expires:	03/31/2013
		Bottle No.:	0138

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:30D		
Control 1 EC	0.099%	11:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	11:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:31D		
Control 2 EC	0.099%	11:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	11:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:33D		
Control 3 EC	0.099%	11:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:34D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OHARE


First Name: BRYAN

MI: F

Signature: _____

Badge No.: 96

Date: 04/04/2012

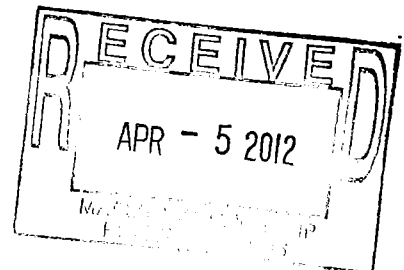

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARXA-0069
Location:	MARLBORO TWP. POLICE	
Calibration File No.:	00261	Calib. Date: 11/01/2011
Certification File No.:	00262	Calib. No.: 00015
Linearity File No.:	00263	Cert. Date: 11/01/2011
Solution File No.:	00299	Cert. No.: 00008
Sequential File No.:	00299	Lin. Date: 11/01/2011
		Lin. No.: 00010
		Soln. Date: 03/07/2012
		Soln. No.: 00066
		File Date: 03/07/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0162
Solution Control Lot:	11C088	Expires: 03/31/2013
		Bottle No.: 0132

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	15:58S		
Control 1 EC	0.099%	15:59S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:00S		
Control 2 EC	0.098%	16:00S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:01S		
Control 3 EC	0.099%	16:02S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	16:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:02S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OHARE

First Name: BRYAN

MI: F

Signature: _____

Sgt. [Signature] #0096

Badge No.: 96

Date: 03/07/2012

MAR 11 8 2012

**MARLBORO TOWNSHIP
POLICE RECORDS**

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0069
Location: MARLBORO TWP. POLICE
Calibration File No.: 00261 Calib. Date: 11/01/2011 Calib. No.: 00015
Certification File No.: 00262 Cert. Date: 11/01/2011 Cert. No.: 00008
Linearity File No.: 00263 Lin. Date: 11/01/2011 Lin. No.: 00010
Solution File No.: 00287 Soln. Date: 02/08/2012 Soln. No.: 00064
Sequential File No.: 00287 File Date: 02/08/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0162
Control Solution %: 0.100% Expires: 03/31/2013
Solution Control Lot: 11C088 Bottle No.: 0127

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:11S		
Control 1 EC	0.100%	18:12S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	18:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:13S		
Control 2 EC	0.099%	18:13S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	18:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:14S		
Control 3 EC	0.099%	18:15S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	18:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:15S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: OHARE

First Name: BRYAN

MI: F

Signature: _____



Badge No.: 96

Date: 02/08/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0069
Location: MARLBORO TWP. POLICE
Calibration File No.: 00261 Calib. Date: 11/01/2011 Calib. No.: 00015
Certification File No.: 00262 Cert. Date: 11/01/2011 Cert. No.: 00008
Linearity File No.: 00263 Lin. Date: 11/01/2011 Lin. No.: 00010
Solution File No.: 00281 Soln. Date: 01/11/2012 Soln. No.: 00063
Sequential File No.: 00281 File Date: 01/11/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0162
Control Solution %: 0.100% Expires: 03/31/2013
Solution Control Lot: 11C088 Bottle No.: 0131

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:02S		
Control 1 EC	0.099%	18:02S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	18:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:03S		
Control 2 EC	0.097%	18:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	18:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:04S		
Control 3 EC	0.098%	18:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	18:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: OHARE

First Name: BRYAN

MI: F

Signature: _____



Badge No.: 96

Date: 01/11/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0069
Location:	MARLBORO TWP. POLICE		
Calibration File No.:	00261	Calib. Date:	11/01/2011
Certification File No.:	00262	Cert. Date:	11/01/2011
Linearity File No.:	00263	Lin. Date:	11/01/2011
Solution File No.:	00275	Soln. Date:	01/05/2012
Sequential File No.:	00275	File Date:	01/05/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0162
Solution Control Lot:	11C088	Expires:	03/31/2013
		Bottle No.:	0136

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:53S		
Control 1 EC	0.100%	14:54S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:54S		
Control 2 EC	0.099%	14:55S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:56S		
Control 3 EC	0.099%	14:56S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:57S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL # DDUJ P2-066 (4)

Changed By:

Last Name: DENNIS	First Name: MARC	MI: W.
Signature: <u>TPR. I [Signature] #5925</u>	Badge No.: 5925	Date: 01/05/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0069
Location:	MARLBORO TWP. POLICE		
Calibration File No.:	00261	Calib. Date:	11/01/2011
Certification File No.:	00262	Cert. Date:	11/01/2011
Linearity File No.:	00263	Lin. Date:	11/01/2011
Solution File No.:	00275	Soln. Date:	01/05/2012
Sequential File No.:	00275	File Date:	01/05/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0162
Solution Control Lot:	11C088	Expires:	03/31/2013
		Bottle No.:	0136

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:53S		
Control 1 EC	0.100%	14:54S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:54S		
Control 2 EC	0.099%	14:55S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	14:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:56S		
Control 3 EC	0.099%	14:56S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:57S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL # DDUJ P2-066 (144)

Changed By:

Last Name: DENNIS

First Name: MARC

MI: W.

Signature: TPR. I [Signature] #5925

Badge No.: 5925

Date: 01/05/2012