



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

ANDREW J. BRUCK
Acting Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 08/10/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1208 to 0.1221 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 21, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Handwritten signature of Michael Kennedy

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of August, 2021.

Handwritten signature of Notary Karen E. Stahl

Notary

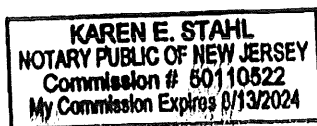

An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



# Alcotest 7110 Calibration Record


**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0069  
Location: MARLBORO TWP. POLICE  
Calibration File No.: 00960 Calib. Date: 08/25/2021 Calib. No.: 00047  
Certification File No.: 00928 Cert. Date: 03/09/2021 Cert. No.: 00036  
Linearity File No.: 00929 Lin. Date: 03/09/2021 Lin. No.: 00040  
Solution File No.: 00958 Soln. Date: 07/25/2021 Soln. No.: 00257  
Sequential File No.: 00960 File Date: 08/25/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0164  
Control Solution %: 0.100% Expires: 10/14/2021  
Solution Control Lot: 19270 Bottle No.: 0496

## Coordinator

Last Name: LUTZ First Name: DENNIS MI: J  
Signature: TP: I Dent 7045 Badge No.: 7045  
Date: 08/25/2021

\*Black Key Temperature Probe Serial.....# DDEEP2-060 (DL)  
\*Digital NIST Temperature Measuring System Serial.....# 200 357 843 (DL)

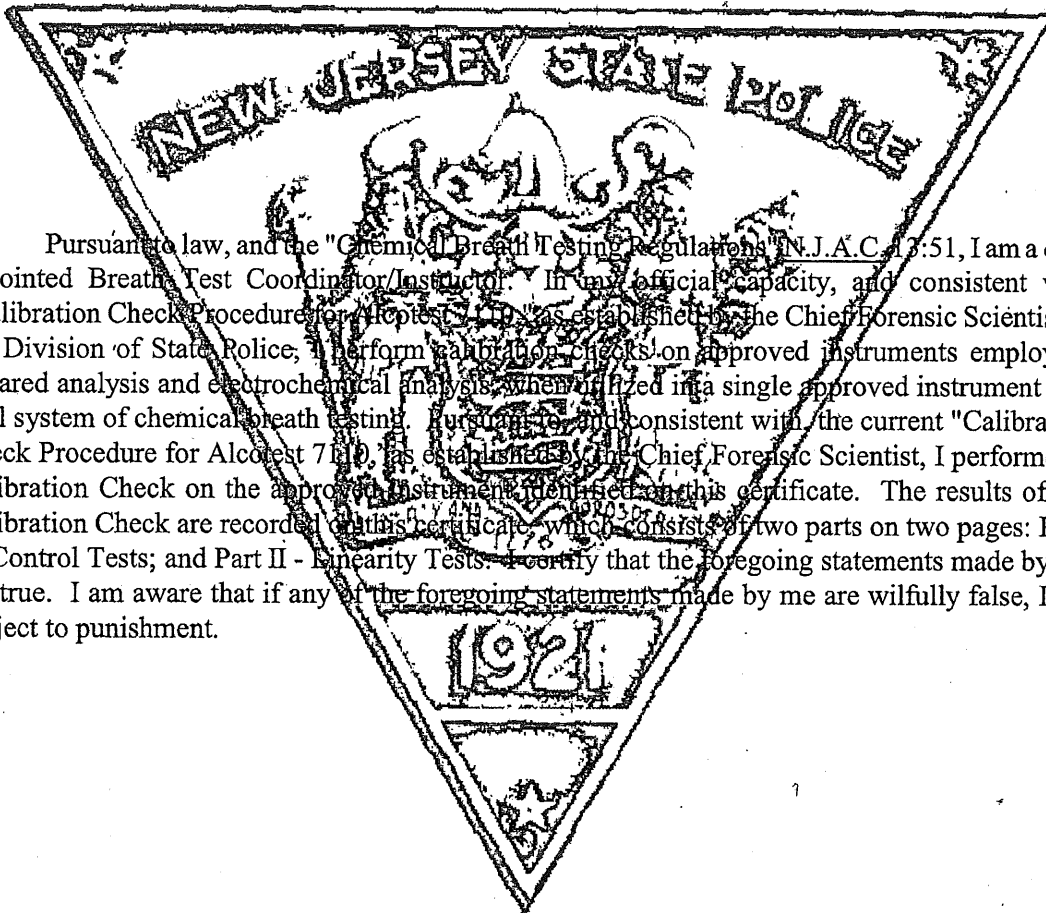

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 17:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0069  
Location: MARLBORO TWP. POLICE  
Calibration File No.: 00960 Calib. Date: 08/25/2021 Calib. No.: 00047  
Certification File No.: 00961 Cert. Date: 08/25/2021 Cert. No.: 00037  
Linearity File No.: 00929 Lin. Date: 03/09/2021 Lin. No.: 00040  
Solution File No.: 00958 Soln. Date: 07/25/2021 Soln. No.: 00257  
Sequential File No.: 00961 File Date: 08/25/2021


Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0164  
Control Solution %: 0.100% Expires: 10/14/2021  
Solution Control Lot: 19270 Bottle No.: 0496

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:01D		
Control 1 EC	0.099%	12:01D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:01D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:02D		
Control 2 EC	0.100%	12:03D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:03D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:03D		
Control 3 EC	0.099%	12:04D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:04D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:05D		

All tests within acceptable tolerance.

### Coordinator

Last Name: LUTZ


Signature: 

Badge No.: 7048

Date: 08/25/2021

MI: J

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 17:27, I am a duly appointed Breath Test Coordinator/Inspector in my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

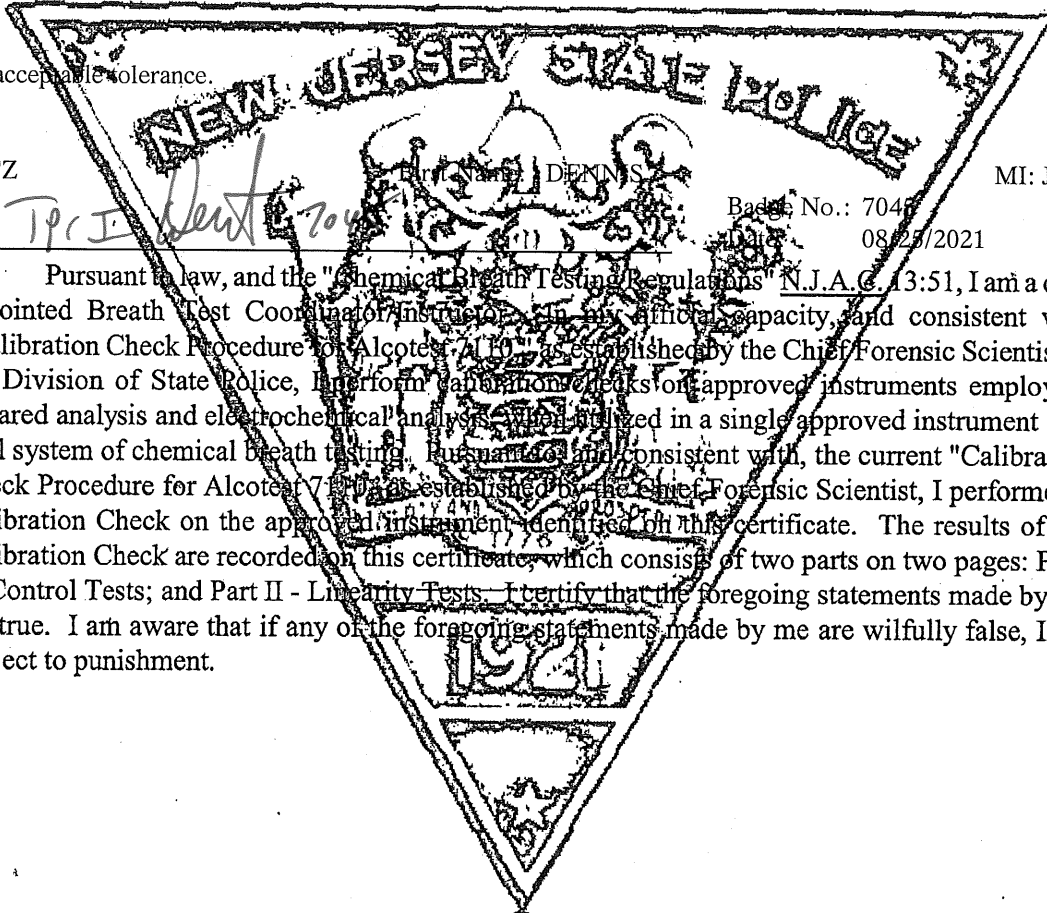

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0069  
Location: MARLBORO TWP. POLICE  
Calibration File No.: 00960 Calib. Date: 08/25/2021 Calib. No.: 00047  
Certification File No.: 00961 Cert. Date: 08/25/2021 Cert. No.: 00037  
Linearity File No.: 00962 Lin. Date: 08/25/2021 Lin. No.: 00041  
Solution File No.: 00958 Soln. Date: 07/25/2021 Soln. No.: 00257  
Sequential File No.: 00962 File Date: 08/25/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDSC S3-0001  
Control Solution %: 0.040% Expires: 11/04/2021  
Solution Control Lot: 19310 Bottle No.: 0885

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0020  
Control Solution %: 0.080% Expires: 11/11/2021  
Solution Control Lot: 19320 Bottle No.: 1337

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDMK S3-0008  
Control Solution %: 0.160% Expires: 12/02/2021  
Solution Control Lot: 19360 Bottle No.: 1320

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:22D		
Control 1 EC	0.040%	12:23D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.039%	12:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:24D		
Control 2 EC	0.040%	12:25D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.039%	12:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:26D		
Control 3 EC	0.080%	12:27D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	12:27D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:28D		
Control 4 EC	0.079%	12:29D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	12:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:30D		
Control 5 EC	0.160%	12:31D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.162%	12:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:32D		
Control 6 EC	0.159%	12:33D	34.1°C	*** TEST PASSED ***
Control 6 IR	0.160%	12:33D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:34D		

All tests within acceptable tolerance.

### Coordinator

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature: \_\_\_\_\_

*TPI I Dent 7045*

Badge No.: 7045

Date: 08/25/2021

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0069
Location:	MARLBORO TWP. POLICE		
Calibration File No.:	00960	Calib. Date:	08/25/2021
Certification File No.:	00961	Cert. Date:	08/25/2021
Linearity File No.:	00962	Lin. Date:	08/25/2021
Solution File No.:	00963	Soln. Date:	08/25/2021
Sequential File No.:	00963	File Date:	08/25/2021
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0164
Solution Control Lot:	21010	Expires:	01/13/2023
		Bottle No.:	0655

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:45D		
Control 1 EC	0.101%	13:46D	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	13:46D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:46D		
Control 2 EC	0.101%	13:47D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	13:47D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:47D		
Control 3 EC	0.101%	13:48D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	13:48D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:49D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDUSP2-080 (DL)

**Changed By:**

Last Name: LUTZ	First Name: DENNIS	MI: J
Signature: <u><i>Tr-I Dent 7045</i></u>	Badge No.: 7045	Date: 08/25/2021

## Alcotest 7110 MKIII-C Calibration NIST-Traceable Digital Thermometer Readings

**Coordinator:**

Tpr I Dennis J Lotz  
Name

7045  
Badge No.

**Location:**

Marlboro Twp. Police  
Agency

AR/A-0069  
Alcotest Serial No.

**Equipment:**

200 357 843  
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDSC 53-0001	10:45 D	11:47 D	33.9°C
0.08%	DDXC 53-0020	10:45 D	11:48 D	34.0°C
0.10%	DDXC 53-0164	10:45 D	11:49 D	34.0°C
0.16%	DDMK 53-0008	10:45 D	11:50 D	34.0°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius  $\pm$  0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

Tpr I Lotz 7045  
Coordinator's Signature

8-25-21  
Date

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: \_\_\_\_\_

Serial Number:

DDSCS3-0001

Certification Date:

6.21.21

Technician:

AM

Re-Certification Due Date:

6.21.22

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: \_\_\_\_\_

Serial Number:

DDXCS3-0020

Certification Date:

6.21.21

Technician:

AM

Re-Certification Due Date:

6.21.22

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: \_\_\_\_\_

Serial Number:

DDMKS3-0008

Certification Date:

6.21.21

Technician:

CR

Re-Certification Due Date:

6.21.22

**Dräger**

**Alcotest 7110 Temperature Probe**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDEEP2-060

Certification Date:

6.21.21

Next Certification Due:

6.21.22

Probe Value:

106

Draeger, Inc.

CR





Calibration complies with ISO/IEC  
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-11349797

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by : VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601,

S/N: 200357843

Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Thermistor Module	A27129	04 Feb 2021	1000451212
Temperature Calibration Bath	A42238		
Temperature Calibration Bath	B01375		
Temperature Probe	5394	21 Feb 2021	C0220030
Temperature Calibration Bath	B16388		
Temperature Probe	5267	21 Feb 2021	C0220028
Temperature Calibration Bath	B3A444		
Thermistor Module	B96381	16 Jul 2020	B9626028
Temperature Probe	5398	16 Jul 2020	B9605083
Thermistor Module	B96382	19 Aug 2020	B9628006
Temperature Probe	5410	13 Sep 2020	B9801031

Certificate Information:

Technician: 420

Procedure: CAL-06

Cal Date: 15 Jun 2020

Cal Due Date: 15 Jun 2022

Test Conditions: 52.44%RH 23.46°C 1018mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		0.000	0.001	Y	-0.05	0.05	0.0087	>4:1
°C	N.A.	N.A.		25.001	25.001	Y	24.951	25.051	0.0087	>4:1
°C	N.A.	N.A.		50.002	50.001	Y	49.952	50.052	0.0087	>4:1
°C	N.A.	N.A.		100.001	99.998	Y	99.951	100.051	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

*Nicol Rodriguez*  
Nicol Rodriguez, Quality Manager

*Marisa Elms*  
Marisa Elms, Technical Manager

Note :

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598  
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.  
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC  
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-11349797

**Traceable® Certificate of Calibration for Digital Thermometer**

**Recalibration:**

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date 15 Jun 2020

**CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598**  
**Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com**

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.  
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/21/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1216 to 0.1232 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 14, 2021.


As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of October, 2019.

[Signature]
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 11/14/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19310

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0485 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 04, 2021.


As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15 day of November, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024

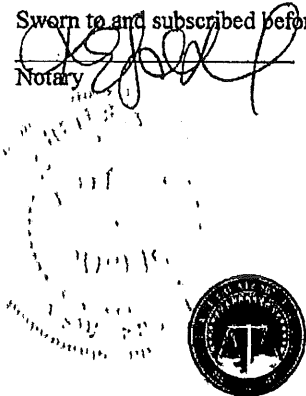

An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 11/20/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19320

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0971 to 0.0985 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 11, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 21 day of November, 2019.

[Signature]
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 12/11/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19360

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1936 to 0.1956 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 02, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18 day of December, 2019.

[Signature]
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 01/28/2021

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 21010

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1212 to 0.1228 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 13, 2023.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 29 day of January, 2021.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110622
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF  
**Traffic and Public Safety**  
*This is to certify that*

**Dennis J. Lutz**

**Breath Test Coordinator/Instructor**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH TESTS PURSUANT TO CHAPTER 140 OF

THE LAWS OF 1964 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 29th DAY OF January

TWO THOUSAND AND Nineteen

*[Signature]*  
COLONEL  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2838 (Rev. 07/07)

DEPARTMENT OF  
**Traffic and Public Safety**  
*This is to certify that*

**Dennis J. Lutz**

**New Jersey State Police**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH TESTS PURSUANT TO CHAPTER 140 OF

THE LAWS OF 1964 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 1st DAY OF October

TWO THOUSAND AND Nine

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 2-3-11	OCPA	Wm Horn
2. 1/24/13	OCPA	Adam Standa
3. 11-23-15	GCPA	M. Gonzalez
4. 4/6/17	LAKEHURST	Adam Standa
5. 8/22/19	NJSP Galloway	Adam Standa
6. 7-19-21	Lakehurst	Adam Standa
7.		
8.		
9.		

S.P. 2838 (Rev. 07/07)



  
**Dräger****Alcotest 7110****CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48854, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

4-4-19ARXA-00129Dräger, Inc. BS

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Dräger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: \_\_\_\_\_

Serial Number:

DDXCS3-0164

Certification Date:

8.12.21

Technician:

AM

Re-Certification Due Date:

8.12.22

**Dräger**

**Alcotest 7110 Temperature Probe**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDUJ P2-080

Certification Date:

8.12.21

Next Certification Due:

8.12.22

Probe Value:

103

Dräger, Inc.

AM