

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0069
Location: MARLBORO TWP. POLICE
Calibration File No.: 00739 Calib. Date: 07/02/2018 Calib. No.: 00038
Certification File No.: 00740 Cert. Date: 07/02/2018 Cert. No.: 00029
Linearity File No.: 00741 Lin. Date: 07/02/2018 Lin. No.: 00033
Solution File No.: 00762 Soln. Date: 10/19/2018 Soln. No.: 00188
Sequential File No.: 00762 File Date: 10/19/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0164
Control Solution %: 0.100% Expires: 09/14/2019
Solution Control Lot: 17290 Bottle No.: 0604

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:01D		
Control 1 EC	0.098%	11:02D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:02D		
Control 2 EC	0.097%	11:03D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04D		
Control 3 EC	0.098%	11:04D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:05D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: RUDITSKY

First Name: DAVID

MI: A

Signature: _____

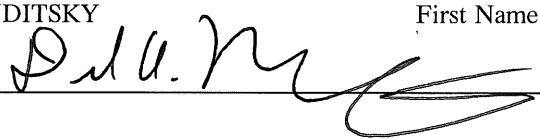

Badge No.: 090

Date: 10/19/2018

