

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARXA-0069
Location:	MARLBORO TWP. POLICE	
Calibration File No.:	00481	Calib. Date: 04/10/2014
Certification File No.:	00482	Calib. No.: 00023
Linearity File No.:	00483	Cert. Date: 04/10/2014
Solution File No.:	00489	Cert. No.: 00015
Sequential File No.:	00489	Lin. Date: 04/10/2014
		Lin. No.: 00018
		Soln. Date: 05/09/2014
		Soln. No.: 00110
		File Date: 05/09/2014
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXC S3-0162
Solution Control Lot:	13K125	Expires: 11/12/2015
		Bottle No.: 1227

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:44D		
Control 1 EC	0.097%	09:45D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:45D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:45D		
Control 2 EC	0.098%	09:46D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:46D		
Control 3 EC	0.098%	09:47D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.097%	09:47D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:47D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Received By**  
**PATROL**  
MAY 13 2014


**Changed By:**

Last Name: UNGRADY

First Name: EDWARD

MI: K

Signature: \_\_\_\_\_

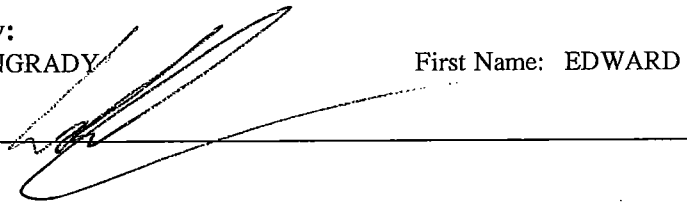

Badge No.: 099

Date: 05/09/2014

