

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0069  
Location: MARLBORO TWP. POLICE  
Calibration File No.: 00681 Calib. Date: 07/27/2017 Calib. No.: 00036  
Certification File No.: 00682 Cert. Date: 07/27/2017 Cert. No.: 00027  
Linearity File No.: 00683 Lin. Date: 07/27/2017 Lin. No.: 00031  
Solution File No.: 00695 Soln. Date: 11/07/2017 Soln. No.: 00170  
Sequential File No.: 00695 File Date: 11/07/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0164  
Control Solution %: 0.100% Expires: 01/30/2019  
Solution Control Lot: 17050 Bottle No.: 1023

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	12:00S		
Control 1 EC	0.101%	12:01S	34.1°C	*** TEST PASSED ***
Control 1 IR	0.101%	12:01S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:02S		
Control 2 EC	0.100%	12:02S	34.1°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:02S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:03S		
Control 3 EC	0.100%	12:04S	34.1°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:04S	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:04S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LOYER

First Name: JOHN

MI: B

Signature: \_\_\_\_\_

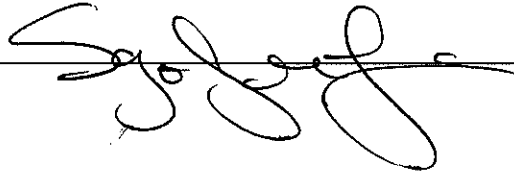

Badge No.: 057

Date: 11/07/2017

