

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0069
Location:	MARLBORO TWP. POLICE		
Calibration File No.:	00657	Calib. Date:	02/02/2017
Certification File No.:	00658	Cert. No.:	00034
Linearity File No.:	00659	Cert. Date:	02/02/2017
Solution File No.:	00670	Lin. Date:	02/02/2017
Sequential File No.:	00670	Lin. No.:	00029
		Soln. Date:	06/02/2017
		Soln. No.:	00160
		File Date:	06/02/2017
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXC S3-0162
Solution Control Lot:	17050	Expires:	01/30/2019
		Bottle No.:	0947

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:16D		
Control 1 EC	0.101%	08:17D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:17D		
Control 2 EC	0.100%	08:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:18D		
Control 3 EC	0.100%	08:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LOYER

First Name: JOHN

MI: B

Signature: _____

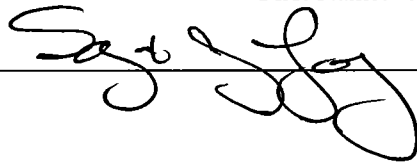

Badge No.: 057

Date: 06/02/2017

