

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0069  
 Location: MARLBORO TWP. POLICE  
 Calibration File No.: 00657 Calib. Date: 02/02/2017 Calib. No.: 00034  
 Certification File No.: 00658 Cert. Date: 02/02/2017 Cert. No.: 00025  
 Linearity File No.: 00659 Lin. Date: 02/02/2017 Lin. No.: 00029  
 Solution File No.: 00675 Soln. Date: 06/22/2017 Soln. No.: 00163  
 Sequential File No.: 00675 File Date: 06/22/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0162  
 Control Solution %: 0.100% Expires: 01/30/2019  
 Solution Control Lot: 17050 Bottle No.: 0823

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:02D		
Control 1 EC	0.102%	18:02D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	18:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:03D		
Control 2 EC	0.100%	18:04D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	18:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:04D		
Control 3 EC	0.101%	18:05D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	18:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:06D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: ARMINIO

First Name: GERALD

MI: A

Signature: \_\_\_\_\_

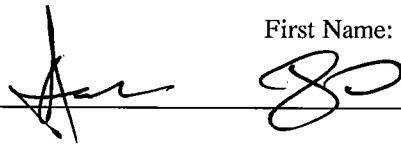

Badge No.: 80

Date: 06/22/2017

