

# Calibrating Unit New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0069  
Location: MARLBORO TWP. POLICE  
Calibration File No.: 00739 Calib. Date: 07/02/2018 Calib. No.: 00038  
Certification File No.: 00740 Cert. Date: 07/02/2018 Cert. No.: 00029  
Linearity File No.: 00741 Lin. Date: 07/02/2018 Lin. No.: 00033  
Solution File No.: 00765 Soln. Date: 11/20/2018 Soln. No.: 00189  
Sequential File No.: 00765 File Date: 11/20/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0164  
Control Solution %: 0.100% Expires: 09/14/2019  
Solution Control Lot: 17290 Bottle No.: 0308

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	07:29S		
Control 1 EC	0.100%	07:29S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	07:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:30S		
Control 2 EC	0.099%	07:31S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	07:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:31S		
Control 3 EC	0.099%	07:32S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	07:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:33S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LOYER

First Name: JOHN

MI: B

Signature: \_\_\_\_\_

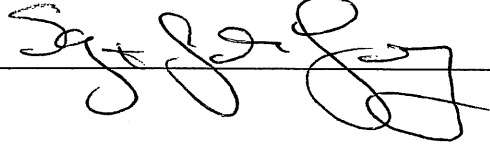

Badge No.: 057

Date: 11/20/2018

