

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0069
Location: MARLBORO TWP. POLICE
Calibration File No.: 00815 Calib. Date: 09/05/2019 Calib. No.: 00042
Certification File No.: 00816 Cert. Date: 09/05/2019 Cert. No.: 00032
Linearity File No.: 00817 Lin. Date: 09/05/2019 Lin. No.: 00036
Solution File No.: 00840 Soln. Date: 12/18/2019 Soln. No.: 00215
Sequential File No.: 00840 File Date: 12/18/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0164
Control Solution %: 0.100% Expires: 09/17/2020
Solution Control Lot: 18290 Bottle No.: 0141

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:53S		
Control 1 EC	0.097%	11:54S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	11:54S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:54S		
Control 2 EC	0.099%	11:55S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	11:55S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:56S		
Control 3 EC	0.099%	11:56S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	11:56S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:57S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: RUDITSKY

First Name: DAVID

MI: A

Signature: _____

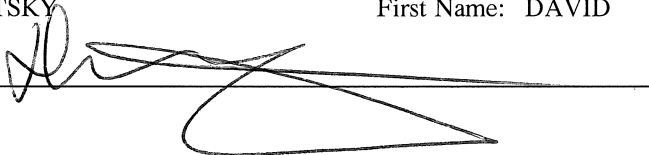

Badge No.: 090

Date: 12/18/2019

