

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0069  
Location: MARLBORO TWP. POLICE  
Calibration File No.: 00657 Calib. Date: 02/02/2017 Calib. No.: 00034  
Certification File No.: 00658 Cert. Date: 02/02/2017 Cert. No.: 00025  
Linearity File No.: 00659 Lin. Date: 02/02/2017 Lin. No.: 00029  
Solution File No.: 00670 Soln. Date: 06/02/2017 Soln. No.: 00160  
Sequential File No.: 00670 File Date: 06/02/2017

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0162  
Control Solution %: 0.100% Expires: 01/30/2019  
Solution Control Lot: 17050 Bottle No.: 0947

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:16D		
Control 1 EC	0.101%	08:17D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:17D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:17D		
Control 2 EC	0.100%	08:18D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:18D		
Control 3 EC	0.100%	08:19D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:19D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: LOYER

First Name: JOHN

MI: B

Signature: \_\_\_\_\_

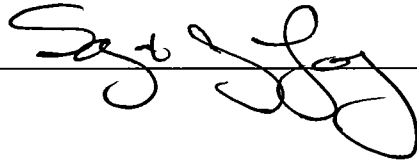

Badge No.: 057

Date: 06/02/2017

